

750 Royal Oaks Drive, Suite 100  
Monrovia, California 91016-3629  
Tel: (626) 386-1100  
Fax: (866) 988-3757  
1 800 566 LABS (1 800 566 5227)

## Laboratory Report

for

Honolulu Board of Water Supply  
630 South Beretania Street  
Public Service Bldg." Room 308  
Honolulu, HI 96843  
Attention: Erwin Kawata  
Fax: 808-550-5018

Date of Issue  
04/21/2022

*Rinda Seddas*  
EUROFINS EATON  
ANALYTICAL, LLC



Utah ELCP CA00006

DEB: Debbie L Frank  
Project Manager

Report: 996836  
Project: RED-HILL  
Group: Weekly TPH-8015\_RED-HILL (2022) - EMAX

\* Accredited in accordance with TNI 2016 and ISO/IEC 17025:2017.

\* Laboratory certifies that the test results meet all TNI 2016 and ISO/IEC 17025:2017 requirements unless noted under the individual analysis.

\* As applicable, this report consists of the cover page, State Certification List, ISO 17025 Accredited Method List, Acknowledgement of Samples Received, Comments, Hits Report, Data Report, QC Summary, QC Report and Regulatory Forms.

\* Test results relate only to the sample(s) tested.

\* Test results apply to the sample(s) as received, unless otherwise noted in the comments report (ISO/IEC 17025:2017).

\* This report shall not be reproduced except in full, without the written approval of the laboratory.

\* This report includes ISO/IEC 17025 and non-ISO 17025 accredited methods.

## STATE CERTIFICATION LIST

State	Certification Number	State	Certification Number
Alabama	41060	Montana	Cert 0035
Arizona	AZ0778	Nebraska	NE-OS-21-13
Arkansas	CA00006	Nevada	CA00006
California	2813	New Hampshire *	2959
Colorado	CA00006	New Jersey *	CA 008
Connecticut	PH-0107	New Mexico	CA00006
Delaware	CA 006	New York *	11320
Florida *	E871024	North Carolina	06701
Georgia	947	North Dakota	R-009
Guam	21-008R	Ohio - 537.1	87786
Hawaii	CA00006	Oregon *	4034
Idaho	CA00006	Pennsylvania *	68-00565
Illinois	200033	Puerto Rico	CA00006
Indiana	C-CA-01	Rhode Island	LAO00326
Iowa – Asbestos	413	South Carolina	87016
Kansas *	E-10268	South Dakota	CA11320
Kentucky	90107	Tennessee	TN02839
Louisiana *	LA008	Texas *	T104704230-20-18
Maine	CA00006	Utah (Primary AB) *	CA00006
Maryland	224	Vermont	VT0114
Marianas Islands	MP0004	Virginia *	460260
Massachusetts	M-CA006	Washington	C838
Michigan	9906	EPA Region 5	CA00006
Mississippi	CA00006	Los Angeles County Sanitation Districts	10264

\* NELAP/TNI Recognized Accreditation Bodies

ISO/IEC 17025:2017 Accredited Method List

The test listed below are accredited and met the requirements of ISO/IEC 17025 as verify by A2LA.

Refer to our certificates and scope of accreditations (no. 5890-1 and 5890-2) found at:

<https://www.eurofinsus.com/Eaton>

Test(s)	Method(s)	Potable Water *	Waste Water
Enterococci	Enterolert	x	x
Escherichia coli (Enumeration)	SM 9221 B.1 SM 9221 F	x	
Fecal Coliform (P/A and Enumeration)	SM 9221 C (MTF/EC), SM 9221 E (MTF/EC)	x	x
Fecal Streptococci and Enterococci	SM 9230 B	x	x
Heterotrophic Bacteria	SM 9215 B	x	
Legionella	Legiolert®	x	
Pseudomonas aeruginosa	Idexx Pseudalert	x	
Total Coliform (P/A and Enumeration)	SM 9221A, SM 9221B, SM 9221 C	x	x
Total Coliform, Total Coliform with Chlorine Present	SM 9221 B	x	x
Total Coliform/E. coli (P/A and Enumeration, Idexx Colilert, Idexx Colilert 18, Colisure)	SM 9223	x	
Total Microcystins and Nodularins	EPA 546	X	
Yeast and Mold	SM 9610	x	
1,2,3-Trichloropropane (TCP) at 5 PPT	CA SRL 524M-TCP	x	
1,4-Dioxane	EPA 522	x	
2,3,7,8-TCDD	Modified EPA 1613 B	x	
Acrylamide	+ LCMS 2440)	x	
Algal Toxins/Microcys in	+ LCMS 3570	x	
Alkalinity	SM 2320B	x	x
Ammonia	EPA 350.1, SM 4500-NH3 H		x
Asbestos	EPA 100.2	x	x
Bicarbonate Alkalinity as HCO3	SM 2330 B	x	x
BOD/CBOD	SM 5210 B		x
Bromate	+ LCMS- 2447	x	
Carbonate as CO3	SM 2330 B	x	x
Carbonyls	EPA 556	x	x
Chemical Oxygen Demand	EPA 410.4, SM 5220D		x
Chlorinated Acids	EPA 515.4	x	
Chlorine Dioxide	Palin Test Chlordio X Plus, SM 4500-CLO2 D	x	
Chlorine, Free, Combined, Total Residual, Chloramines	SM 4500-Cl G	x	
Color	SM2120B	x	
Conductivity	EPA 120.1, SM 2510B	x	x
Corrosivity (Langelier Index), Carbonate as CO3, Hydroxide as OH Calculated	SM 2330 B	x	
Cyanide (Amenable)	SM 4500-CN G	x	x
Cyanide (Free)	SM 4500CN F	x	x
Cyanide (Total)	EPA 335.4	x	x
Cyanogen Chloride (Screen)	+ 335 Mod (WC-24467)	x	
Diquat and Paraquat	EPA 549.2	x	
DBP and HAA	SM 6251 B	x	
Dissolved Organic Carbon	SM 5310 C	x	
Dissolved Oxygen	SM 4500-O G		x
EDB/DCBP/TCP	EPA 504.1	x	
EDB/DBCP and Disinfection Byproducts	EPA 551.1	x	
EDTA and NTA	+ WC-2454	x	
Endothall	EPA 548.1, +(LCMS-2445)	x	
Fluoride	SM 4500F C	x	x
Glyphosate	EPA 547	x	
Glyphosate and AMPA	+ LCMS-3618	x	
Gross Alpha and Gross Beta	EPA 900.0	x	x

Test(s)	Method(s)	Potable Water *	Waste Water
Gross Alpha coprecipitation	SM 7110 C	x	x
Hardness	SM 2340 B	x	x
Hexavalent Chromium	EPA 218.6,	x	x
Hexavalent Chromium	EPA 218.7,	x	
Hexavalent Chromium	SM 3500-Cr B		x
Inorganic Anions and DBPs	EPA 300.0	x	x
Norganic Anions and DBPs	EPA 300.1	x	
Kjeldahl Nitrogen	EPA 351.2		x
Metals	EPA 200.7, EPA200.8	x	x
Nitrosamines	EEA-Agilent 521.1 (GCMS-24250)	x	
Nitrate/Nitrite Nitrogen	EPA 353.2	x	x
Odor	SM2150B	x	
Organohalide Pesticides and PCB	EPA 505	x	
Ortho Phosphate	SM 4500P E	x	
Oxyhalides Disinfect ion Byproducts	EPA 317.0	x	
Perchlorate	EPA 331.0	x	
Perchlorate (Low and High Levels)	EPA 314.0	x	
Perfluorinated Alkyl Acids	EPA 533, EPA 537, EPA 537.1	x	
PPCP and EDC	+ LCMS-2443	x	
pH	EPA 150.1 SM 4500-H+ B	x	x
Phenolics – Low Level	+WC 2493 (EPA 420.2 and EPA 420.4 MOD)	x	x
Phenylurea Pesticides/Herbicides	+ LCMS-2448	x	
Radium-226, Radium-228	GA Tech (Rad-2374)	x	
Radon-222	SM 7500RN	x	
Residue (Filterable)	SM 2540C	x	x
Residue (Non-Filterable)	SM 2540D		x
Residue (Total)	SM 2540B		x
Residue (Volatile)	EPA 160.4		x
Semi-Volatile Compounds	EPA 525.2	x	
Silica	SM 4500-SiO2 C	x	x
Sulfide	SM 4500-S D		x
Sulfite	SM 4500-SO3 B	x	x
Surfactants	SM 5540C	x	x
Taste and Odor	SM 6040 E	x	
Total Organic Carbon	SM 5310 C	x	x
Total Phenols	EPA 420.1		x
Total Phenols	EPA 420.4	x	x
Triazine Pesticides and their Degradates	+ LCMS-3617	x	
Turbidity	EPA 180.1	x	x
Uranium by ICP/MS	EPA 200.8	x	
UV 254 Organic Constituents	SM 5910B	x	
VOCs	EPA 524.2	x	
VOCs	+(GCMS 2412) by EPA 524.2 modified	x	

(\*) includes: Bottled Water, Drinking Water and Water as Component of Food & Beverage.

(+) In-House Method

**Acknowledgement of Samples Received**

Addr: **Honolulu Board of Water Supply**  
630 South Beretania Street  
Public Service Bldg." Room 308  
Honolulu, HI 96843

Attn: Erwin Kawata  
Phone: 808-748-5091

Client ID: HONOLULU  
Folder #: 996836  
Project: RED-HILL  
Sample Group: Weekly TPH-8015\_RED-HILL (2022)  
- EMAX  
Project Manager: Debbie L Frank  
Phone: (626) 386-1149  
PO #: C20525101 exp 05312023


The following samples were received from you on **April 05, 2022 at 1231**. They have been scheduled for the tests listed below each sample. If this information is incorrect, please contact your service representative. Thank you for using Eurofins Eaton Analytical, LLC.

Sample #	Sample ID	Sample Date
202204050426	HALAWA WELLS P2 (331-024-WL064)	04/04/2022 1007
	SDWIS PWSID: HI0000331 SDWIS FACILITY ID: WL064 SDWIS SAMPLE POINT ID: 024	
	(SUB)Gas Fraction Hydrocarbons	TPH 8015 Diesel and Motor Oil

**Test Description**







Eurolns Analytical

# INTERNAL CHAIN OF CUSTODY RECORD

SAMPLE TEMP RECEIVED: \_\_\_\_\_  
Note: If samples are out of temperature range, let the ASMs know. ASMs will determine whether to proceed with analysis or not.  
SAMPLES REC'D DAY OF COLLECTION? Yes / No

IR Gun ID = 649A (Observation = 4.0 °C) (Corr. Factor = 0.3 °C) (Final = 3.7 °C)  
TYPE OF ICE: Real  Synthetic  No Ice  Frozen  Partially Frozen  Thawed  N/A

METHOD OF SHIPMENT: Pick-Up / Walk-In / FedEX / UPS / DHL / Area Fast / Top Line / Other: \_\_\_\_\_

### Compliance Acceptance Criteria:

- 1) Chemistry: >0, ≤6°C, not frozen (NELAP) (If received after 24 hrs of sample collection)
- 2) Microbiology, Distribution: < 10°C, not frozen (can be ≥10°C if received on ice the same day as sample collection, within 8 hours)
- 3) Microbiology, Surface Water: < 10°C (if received after 2 hours of sample collection)

If out of temperature range for both Chemistry and Microbiology samples and temperature does not confirm, then measure the temperature of each quadrant and record each temperature of the quadrants

1 = (Observation = _____ °C) (Corr. Factor = _____ °C) (Final = _____ °C)	2 = (Observation = _____ °C) (Corr. Factor = _____ °C) (Final = _____ °C)
3 = (Observation = _____ °C) (Corr. Factor = _____ °C) (Final = _____ °C)	4 = (Observation = _____ °C) (Corr. Factor = _____ °C) (Final = _____ °C)

- 4) Dioxin (1613 or 2,3,7,8 TCDD): must be between 0-4 °C, not frozen (if received after 24 hrs of sample collection)
- 5) pH Check, Manufacturer: \_\_\_\_\_ Lot Number: \_\_\_\_\_ pH strip type: 0 - 14 or \_\_\_\_\_ Expiration Date: \_\_\_\_\_ Results: \_\_\_\_\_
- 6) Chlorine check, Manufacturer: Sansafe, Lot No.: \_\_\_\_\_ Expiration Date: \_\_\_\_\_ Results: \_\_\_\_\_

- 7) VOA and Radon Headspace: \_\_\_\_\_  
No Samples with Headspace: \_\_\_\_\_  
Samples with Headspace (see below): \_\_\_\_\_

Headspace Documentation (use additional VOC and Radon Internal COFC for additional bottles)  
Exempt from headspace concerns: Methods 515.4, HAA(621,662), 605, SPME, @CH, 632LCMS, 669, 639, Anatoxin, LCMS methods using 40 ml vials, international clients:

Samp ID	Bottle #	None/<8	>6mm	Test	Samp ID	Bottle #	None/<8	>6mm	Test


Note Sample IDs which have dissimilar headspace (i.e. potential sampling errors): \_\_\_\_\_

RECEIVED BY: \_\_\_\_\_ SIGNATURE: G REITNER PRINT NAME: \_\_\_\_\_

COMPANY/TITLE: Eurofins Ecoln Analytical DATE: 04.05.2022 TIME: 12:31

SAMPLES CHECKED AGAINST COC BY: \_\_\_\_\_ SIGNATURE: \_\_\_\_\_ PRINT NAME: \_\_\_\_\_

COMPANY/TITLE: Eurofins Ecoln Analytical DATE: \_\_\_\_\_ TIME: \_\_\_\_\_



Eaton Analytical

# INTERNAL CHAIN OF CUSTODY RECORD

EEA Folder Number:  

IR Gun ID = 619A (Observation = 3.5 °C) (Corr.Factor = 0.3 °C) (Final = 3.2 °C)

TYPE OF ICE: Real  Synthetic  No Ice  CONDITION OF ICE: Frozen  Partially Frozen  Thawed  N/A

METHOD OF SHIPMENT: Pick-Up / Walk-In (FedEx) UPS / DHL / Area Fast / Top Line / Other:

### Compliance Acceptance Criteria:

- 1) Chemistry: >0, ≤6°C, not frozen (NELAP) (If received after 24 hrs of sample collection)
- 2) Microbiology, Distribution: < 10°C, not frozen (can be ≥10°C if received on ice the same day as sample collection, within 8 hours)
- 3) Microbiology, Surface Water: < 10°C (if received after 2 hours of sample collection)

If out of temperature range for both Chemistry and Microbiology samples and temperature does not confirm, then measure the temperature of each quadrant and record each temperature of the quadrant

1 - (Observation) °C	(Corr.Factor) °C	(Final) °C	2 - (Observation) °C	(Corr.Factor) °C	(Final) °C
3 - (Observation) °C	(Corr.Factor) °C	(Final) °C	4 - (Observation) °C	(Corr.Factor) °C	(Final) °C

4) Dioxin (1613 or 2,3,7,8 TCDD): must be between 0-4 °C, not frozen (if received after 24 hrs of sample collection)

5) pH Check, Manufacturer:  Lot Number:  pH strip type: 0 - 14 or  Expiration Date  Results:

6) Chlorine check, Manufacturer: Sansafe, Lot No.:  Expiration Date:  Results:

7) VOA and Radon Headspace:  No Samples with Headspace:  Samples with Headspace (see below):

Headspace Documentation (use additional VOC and Radon Internal COFC for additional bottles)  
 Exempt from headspace concerns: Methods 816.4, HAA(8281,882), 806, SPME, @CH, 821LCH8, 888, 838, Anstoxin, LCMS methods using 40 ml vials, international clients:

Sample ID	Bottle #	None/<8	>8mm	Test	Sample ID	Bottle #	None/<8	>8mm	Test

Note Sample IDs which have dissimilar headspace (i.e. potential sampling errors):

RECEIVED BY: GA SIGNATURE: G. REINER PRINT NAME: Eurofins Eaton Analytical DATE: 04.05.2022 TIME: 12:31

SAMPLES CHECKED AGAINST COG BY:   SIGNATURE:   PRINT NAME: Eurofins Eaton Analytical DATE:   TIME:

ORIGIN ID: HKA (808) 748-5840  
 BWS CHEM LAB  
 HONOLULU BOARD OF WATER SUPPLY  
 630 S. BERETANIA ST.  
 CHEMICAL LABORATORY  
 HONOLULU, HI 96843  
 UNITED STATES US

SHIP DATE: 04APR22  
 ACTWGT: 78.00 LB  
 CAD: 100205419/NET4460


BILL RECIPIENT

TO

EUROFINS EATON ANALYTICAL, INC  
 750 ROYAL OAKS DR  
 SUITE 100

MONROVIA CA 91016  
 (626) 386-1178  
 REF: PO: DEPT:

56D.J2/BDF9/FE4A




1 of 2

TRK# 7764 8792 7214  
 0201  
 ## MASTER ##

TUE - 05 APR 10:30A  
 PRIORITY OVERNIGHT

WZ WHPA

CA-US 91016  
 BUR



**After printing this label:**

1. Use the 'Print' button on this page to print your label to your laser or inkjet printer.
2. Fold the printed page along the horizontal line.
3. Place label in shipping pouch and affix it to your shipment so that the barcode portion of the label can be read and scanned.

**Warning:** Use only the printed original label for shipping. Using a photocopy of this label for shipping purposes is fraudulent and could result in additional billing charges, along with the cancellation of your FedEx account number. Use of this system constitutes your agreement to the service conditions in the current FedEx Service Guide, available on fedex.com. FedEx will not be responsible for any claim in excess of \$100 per package, whether the result of loss, damage, delay, non-delivery, misdelivery, or misinformation, unless you declare a higher value, pay an additional charge, document your actual loss and file a timely claim. Limitations found in the current FedEx Service Guide apply. Your right to recover from FedEx for any loss, including intrinsic value of the package, loss of sales, income interest, profit, attorney's fees, costs, and other forms of damage whether direct, incidental, consequential, or special is limited to the greater of \$100 or the authorized declared value. Recovery cannot exceed actual documented loss. Maximum for items of extraordinary value is \$1,000, e.g. jewelry, precious metals, negotiable instruments and other items listed in our Service Guide. Written claims must be filed within strict time limits, see current FedEx Service Guide.



ORIGIN ID:HIKA (808) 748-5840  
 BWS CHEM LAB  
 HONOLULU BOARD OF WATER SUPPLY  
 630 S. BERETANIA ST  
 CHEMICAL LABORATORY  
 HONOLULU, HI 96843  
 UNITED STATES US

SHIP DATE: 04APR22  
 ACTWGT: 58.00 LB  
 CAD: 100205419/NET4460


BILL RECIPIENT

TO

EUROFINS EATON ANALYTICAL, INC  
 750 ROYAL OAKS DR  
 SUITE 100  
 MONROVIA CA 91016

REF: (626) 386-1178  
 INV. PO. DEPT.

56DJ2/BDF9/FE4A



2 of 2

MPS# 7764 8792 7832  
 0263


Mstr# 7764 8792 7214

0201

TUE - 05 APR 10:30A  
 PRIORITY OVERNIGHT

**WZ WHPA**

CA-US  
 91016  
 BUR



**After printing this label:**

1. Use the 'Print' button on this page to print your label to your laser or inkjet printer.
2. Fold the printed page along the horizontal line.
3. Place label in shipping pouch and affix it to your shipment so that the barcode portion of the label can be read and scanned.

**Warning:** Use only the printed original label for shipping. Using a photocopy of this label for shipping purposes is fraudulent and could result in additional billing charges, along with the cancellation of your FedEx account number. Use of this system constitutes your agreement to the service conditions in the current FedEx Service Guide, available on fedex.com. FedEx will not be responsible for any claim in excess of \$100 per package, whether the result of loss, damage, delay, non-delivery, misdelivery, or misinformation, unless you declare a higher value, pay an additional charge, document your actual loss and file a timely claim. Limitations found in the current FedEx Service Guide apply. Your right to recover from FedEx for any loss, including intrinsic value of the package, loss of sales, income interest, profit, attorney's fees, costs, and other forms of damage whether direct, incidental, consequential, or special is limited to the greater of \$100 or the authorized declared value. Recovery cannot exceed actual documented loss. Maximum for items of extraordinary value is \$1,000, e.g. jewelry, precious metals, negotiable instruments and other items listed in our Service Guide. Written claims must be filed within strict time limits, see current FedEx Service Guide.

Tel: (626) 386-1100  
Fax: (866) 988-3757  
1 800 566 LABS (1 800 566 5227)

**Laboratory Comments**

**Report:** 996836  
**Project:** RED-HILL  
**Group:** Weekly TPH-8015\_RED-HILL (2022)  
- EMAX

Honolulu Board of Water Supply  
Erwin Kawata  
630 South Beretania Street  
Public Service Bldg." Room 308  
Honolulu, HI 96843

---

**Folder Comments**

Analytical results for TPH 8015 Gas, Diesel and Motor Oil are submitted by Emax Laboratories, Inc. Torrance, CA



Eaton Analytical

Tel: (626) 386-1100  
Fax: (866) 988-3757  
1 800 566 LABS (1 800 566 5227)

**Laboratory Hits**

**Report:** 996836  
**Project:** RED-HILL  
**Group:** Weekly TPH-8015\_RED-HILL (2022)  
- EMAX

**Honolulu Board of Water Supply**  
Erwin Kawata  
630 South Beretania Street  
Public Service Bldg." Room 308  
Honolulu, HI 96843

Samples Received on:  
04/05/2022 1231

---

Analyzed	Analyte	Sample ID	Result	HI Limit	Units	MRL
----------	---------	-----------	--------	----------	-------	-----

---

**SUMMARY OF POSITIVE DATA ONLY**

Tel: (626) 386-1100  
 Fax: (626) 988-3757  
 1 800 566 LABS (1 800 566 5227)

Laboratory Data

**Report:** 996836  
**Project:** RED-HILL  
**Group:** Weekly TPH-8015\_RED-HILL (2022)  
 - EMAX

**Honolulu Board of Water Supply**  
 Erwin Kawata  
 630 South Beretania Street  
 Public Service Bldg." Room 308  
 Honolulu, HI 96843

Samples Received on:  
 04/05/2022 1231

Prepped	Analyzed	Prep Batch	Analytical Batch	Method	Analyte	Result	Units	MRL	Dilution
<b><u>HALAWA WELLS P2 (331-024-WL064) (202204050426)</u></b>						<b>Sampled on 04/04/2022 1007</b>			
Facility ID: WL064									
Sample Point ID: 024									
PWSID: HI0000331									
<b>SW 8015B - (SUB)Gas Fraction Hydrocarbons</b>									
04/06/22	04/06/22 17:20			(SW 8015B)	(SUB)Gas Fraction Hydrocarbons	ND	mg/L	0.02	1
<b>SW 8015B - TPH 8015 Diesel and Motor Oil</b>									
04/06/22	04/07/22 18:42			(SW 8015B)	TPH Diesel	ND	mg/L	0.024	1
04/06/22	04/07/22 18:42			(SW 8015B)	TPH Motor Oil	ND	mg/L	0.047	1

Rounding on totals after summation.  
 (c) - indicates calculated results. Analysis is a calculated result. Reported results are not rounded until the final step before reporting. Therefore methods that use a test result with further calculation may have slight differences in final result than the component analyses.



3051 Fujita Street  
Torrance, CA 90505  
Tel: (310)-618-8889

Date: 04-19-2022  
EMAX Batch No.: 22D027

Attn: Jackie Contreras

Eurofins Eaton Analytical  
750 Royal Oaks Dr., Suite 100  
Monrovia, CA 91016-3629

Subject: Laboratory Report  
Project: 996836

Enclosed is the Laboratory report for samples received on 04/06/22.  
The data reported relate only to samples listed below :

Sample ID	Control #	Col Date	Matrix	Analysis
202204050426	D027-01	04/04/22	WATER	TPH GASOLINE TPH DIESEL & MOTOR OIL

The results are summarized on the following pages.

Please feel free to call if you have any questions concerning these results.

Sincerely yours,


Caspar J. Pang  
Laboratory Director

This report is confidential and intended solely for the use of the individual or entity to whom it is addressed. This report shall not be reproduced except in full or without the written approval of EMAX.

EMAX certifies that results included in this report meets all TNI & DOD requirements unless noted in the Case Narrative.

NELAP Accredited Certificate Number CA002912021-19  
ANAB Accredited DoD ELAP and ISO/IEC 17025 Certificate Number L2278 Testing  
California ELAP Accredited Certificate Number 2672





Eaton Analytical

Ship To:  
EMAX Laboratories, Inc.  
3051 Fujita St.  
Torrance, CA 90505

Phone: 310-618-8889 Fax: 310-618-0818

Folder #: 996836 Report Due: 04/12/2022

Sample ID: 202204050426 Client Sample ID for reference onl: HALAWA WELLS P2 (331-024-WL064)

Sample type: Sample Event: Sample ID: Static ID:

Method: SW 8015B EPA 5030C EPA 3550B Analysis Requested: (SUB)Gas Fraction Hydrocarbons TPH 8015 Diesel and Motor Oil

Submittal Form

Date: 4/6/2022

\*REPORTING REQUIREMENTS: Do Not Combine Reports with any other samples submitted under different Folder Numbers! Report & Invoice must have the Folder # 996836 Job # 1000014

Report all quality control data according to Method. Include dates analyzed. Date extracted (if extracted) and Method reference on the report. Results must have Complete data & QC with Approval Signature.

Reports: Jackie Contreras Sub-Contracting Administrator  
EMAIL TO: Eaton-MonroviaSubContract@eurofins.com  
Eurofins Eaton Analytical, LLC 750 Royal Oaks Drive, Suite 100, Monrovia, CA 91016  
Phone (626) 386-1165 Fax (626) 386-1122  
Invoices to: Eurofins Eaton Analytical, LLC  
Accounts Payable 2425 New Holland Pike, Lancaster, PA 17605

Provide in each Report the Specified State/Certification # and Exp Date for requested tests + matrix.

Samples from: HAWAII

EMAX - 4 or 3 containers per sample for MS/MSD batch QC. Low level RL reporting only

Sample Date & Time Matrix Clip Code PWSID  
04/04/22 1007 DW JLS

Relinquished by: [Signature] Sample Control Date: 4/6/22 Time: 12:11  
Received by: [Signature] Date: 4/6/22 Time: 12:11  
Relinquished by: Sample Control Date: Date Time:  
Received by: Date Date Time:

NOTIFICATION REQUIRED IF RECEIVED OUTSIDE OF 0-6 CELSIUS

An Acknowledgement of Receipt is requested to attn: Jackie Contreras

TEMP ① 0.5/0.7 ② 0.4/0.6

Type of Delivery <input type="checkbox"/> Fedex <input type="checkbox"/> UPS <input type="checkbox"/> GSO <input type="checkbox"/> Others	Airbill / Tracking Number	ECN <u>22D027</u>
<input type="checkbox"/> EMAX Courier <input checked="" type="checkbox"/> Client Delivery		Recipient <u>Alan RAMOS</u>
		Date <u>4/6/22</u> Time <u>12:11</u>

**COC INSPECTION**

<input checked="" type="checkbox"/> Client Name	<input checked="" type="checkbox"/> Client PM/FC	<input type="checkbox"/> Sampler Name	<input checked="" type="checkbox"/> Sampling Date/Time	<input checked="" type="checkbox"/> Sample ID	<input checked="" type="checkbox"/> Matrix
<input checked="" type="checkbox"/> Address	<input checked="" type="checkbox"/> Tel # / Fax #	<input type="checkbox"/> Courier Signature	<input checked="" type="checkbox"/> Analysis Required	<input type="checkbox"/> Preservative (if any)	<input type="checkbox"/> TAT
Safety Issues (if any)	<input type="checkbox"/> High concentrations expected	<input type="checkbox"/> From Superfund Site	<input type="checkbox"/> Rad screening required		

Note: \_\_\_\_\_


**PACKAGING INSPECTION**

Container <u>* correction</u>	<input checked="" type="checkbox"/> Cooler	<input type="checkbox"/> Box	<input type="checkbox"/> Other
Condition <u>factor</u>	<input type="checkbox"/> Custody Seal	<input type="checkbox"/> Intact	<input type="checkbox"/> Damaged
Packaging <u>tar</u>	<input checked="" type="checkbox"/> Bubble Pack	<input type="checkbox"/> Styrofoam	<input type="checkbox"/> Popcorn
Temperatures (Cool. ≤6 °C but not frozen)	<input checked="" type="checkbox"/> Cooler 1 <u>10.5/0.7</u> °C	<input checked="" type="checkbox"/> Cooler 2 <u>20.4/0.6</u> °C	<input type="checkbox"/> Cooler 3 _____ °C
Thermometer: <u>A - S/N 210533479</u>	<input type="checkbox"/> Cooler 6 _____ °C	<input type="checkbox"/> Cooler 7 _____ °C	<input type="checkbox"/> Cooler 4 _____ °C
	<input type="checkbox"/> Cooler 8 _____ °C	<input type="checkbox"/> Cooler 9 _____ °C	<input type="checkbox"/> Cooler 5 _____ °C
		<input type="checkbox"/> Cooler 10 _____ °C	

Comments:  Temperature is out of range. PM was informed IMMEDIATELY.

Note: \_\_\_\_\_

**DISCREPANCIES**

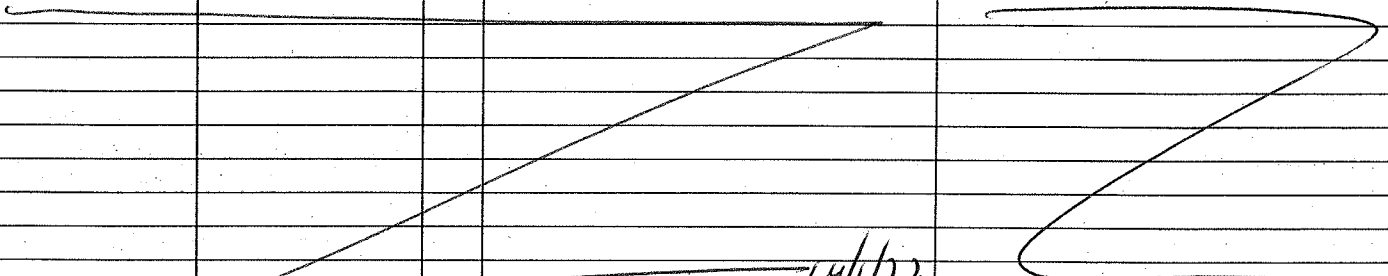LabSampleID	LabSampleContainerID	Code	ClientSample Label ID / Information	Corrective Action
1	A-9	D1	Jet Fuel S not mentioned in COC	RS
1	3	D2	4/6/22	
				

pH holding time requirement for water samples is 15 mins. Water samples for pH analysis are received beyond 15 minutes from sampling time.

MS 4/7/22

**NOTES/OBSERVATIONS:**

SAMPLE MATRIX IS DRINKING WATER?  YES  NO

**LEGEND:**

**Code Description- Sample Management**

- D1 Analysis is not indicated in COC
- D2 Analysis mismatch COC vs label
- D3 Sample ID mismatch COC vs label
- D4 Sample ID is not indicated in \_\_\_\_\_
- D5 Container -[improper] [leaking] [broken]
- D6 Date/Time is not indicated in \_\_\_\_\_
- D7 Date/Time mismatch COC vs label
- D8 Sample listed in COC is not received
- D9 Sample received is not listed in COC
- D10 No initial/date on corrections in COC/label
- D11 Container count mismatch COC vs received
- D12 Container size mismatch COC vs received

**Code Description-Sample Management**

- D13 Out of Holding Time
- D14 Bubble is >6mm
- D15 No trip blank in cooler
- D16 Preservation not indicated in \_\_\_\_\_
- D17 Preservation mismatch COC vs label
- D18 Insufficient chemical preservative
- D19 Insufficient Sample
- D20 No filtration info for dissolved analysis
- D21 No sample for moisture determination
- D22 Analysis covered 4/6/22
- D23 \_\_\_\_\_
- D24 \_\_\_\_\_

Continue to next page.

**Code Description-Sample Management**

- R1 Proceed as indicated in  COC  Label
- R2 Refer to attached instruction
- R3 Cancel the analysis
- R4 Use vial with smallest bubble first
- R5 Log-in with latest sampling date and time+1 min
- R6 Adjust pH as necessary
- R7 Filter and preserved as necessary
- R8 Informed client.
- R9 \_\_\_\_\_
- R10 \_\_\_\_\_
- R11 \_\_\_\_\_
- R12 \_\_\_\_\_

**REVIEWS:**

Sample Labeling JHOJIN ZAMORA  
Date 4/6/22

Repleta  
4/6/22

SRF Central  
Date 4/6/22

PM MS  
Date 4/7/22

## REPORTING CONVENTIONS

### DATA QUALIFIERS:

Lab Qualifier	AFCEE Qualifier	Description
J	F	Indicates that the analyte is positively identified and the result is less than RL but greater than MDL.
N		Indicates presumptive evidence of a compound.
B	B	Indicates that the analyte is found in the associated method blank as well as in the sample at above QC level.
E	J	Indicates that the result is above the maximum calibration range or estimated value.
*	*	Out of QC limit.

**Note:** The above qualifiers are used to flag the results unless the project requires a different set of qualification criteria.

### ACRONYMS AND ABBREVIATIONS:

CRDL	Contract Required Detection Limit
RL	Reporting Limit
MRL	Method Reporting Limit
PQL	Practical Quantitation Limit
MDL	Method Detection Limit
DO	Diluted out

### DATES

The date and time information for leaching and preparation reflect the beginning date and time of the procedure unless the method, protocol, or project specifically requires otherwise.

LABORATORY REPORT FOR

EUROFINS EATON ANALYTICAL

996836

METHOD 5030B/8015B  
TOTAL PETROLEUM HYDROCARBONS BY PURGE AND TRAP

SDG#: 22D027

## CASE NARRATIVE

Client : EUROFINS EATON ANALYTICAL

Project: 996836

SDG : 22D027

### METHOD 5030B/8015B TOTAL PETROLEUM HYDROCARBONS BY PURGE AND TRAP

One(1) water sample was received on 04/06/22 to be analyzed for Total Petroleum Hydrocarbons by Purge and Trap in accordance with Method 5030B/8015B and project specific requirements.

#### Holding Time

The sample was analyzed within the prescribed holding time.

#### Calibration

Multi-calibration points were generated to establish initial calibration (ICAL). ICAL was verified using a secondary source (ICV). Continuing calibration (CCV) verifications were carried out on a frequency specified by the project. All calibration requirements were within acceptance criteria. Refer to calibration summary forms of ICAL, ICV and CCV for details. MRL was analyzed as required by the project. Refer to MRL summary form for details.

#### Method Blank

Method blank was prepared and analyzed at the frequency required by the project. For this SDG, one(1) method blank was analyzed. VG55D02B - result was compliant to project requirement. Refer to sample result summary form for details.

#### Lab Control Sample

Lab control sample was prepared and analyzed at a frequency required by the project. For this SDG, one(1) set of LCS/LCD was analyzed. VG55D02L/VG55D02C were within LCS limits. Refer to LCS summary form for details.

#### Matrix QC Sample

Matrix spike sample was prepared and analyzed at a frequency required by the project. For this SDG, one(1) set of MS/MSD was analyzed. Gasoline was within MS QC limits in D026-01M/D026-01S. Refer to Matrix QC summary form for details.

#### Surrogate

Surrogate was added on QC and field samples. All surrogate recoveries were within QC limits. Refer to sample result summary forms for details.

#### Sample Analysis

The sample was analyzed according to prescribed analytical procedures. Results were evaluated in accordance to project requirements. For this SDG, all quality control requirements were met.



LAB CHRONICLE  
TOTAL PETROLEUM HYDROCARBONS BY PURGE AND TRAP

Client : EUROFINS EATON ANALYTICAL  
Project : 996836

SDG NO. : 22D027  
Instrument ID : GCT055

Client Sample ID	Laboratory Sample ID	Dilution Factor	% Moist	WATER		Extraction Date/Time	Sample Data FN	Calibration Data FN	Notes
				Analysis Date/Time	Prep. Batch				
MBLK1W	VG55D02B	1	NA	04/06/2215:29	04/06/2215:29	UD06005A	UD06004A	22VG55D02	Method Blank
LCS1W	VG55D02L	1	NA	04/06/2216:06	04/06/2216:06	UD06006A	UD06004A	22VG55D02	Lab Control Sample (LCS)
LCD1W	VG55D02C	1	NA	04/06/2216:43	04/06/2216:43	UD06007A	UD06004A	22VG55D02	LCS Duplicate
202204050426	D027-01	1	NA	04/06/2217:20	04/06/2217:20	UD06008A	UD06004A	22VG55D02	Field Sample

FN - Filename  
% Moist - Percent Moisture

# **SAMPLE RESULTS**

METHOD 5030B/8015B  
TOTAL PETROLEUM HYDROCARBONS BY PURGE AND TRAP

```

=====
Client      : EUROFINS EATON ANALYTICAL   Date Collected: 04/04/22 10:07
Project     : 996836                     Date Received: 04/06/22
Batch No.   : 22D027                     Date Extracted: 04/06/22 17:20
Sample ID   : 202204050426              Date Analyzed: 04/06/22 17:20
Lab Samp ID: D027-01                     Dilution Factor: 1
Lab File ID: UD06008A                    Matrix: WATER
Ext Btch ID: 22VG55D02                  % Moisture: NA
Calib. Ref.: UD06004A                   Instrument ID: 55
=====

```

PARAMETERS	RESULTS (mg/L)	RL (mg/L)	MDL (mg/L)	
GASOLINE	ND	0.020	0.010	
SURROGATE PARAMETERS	RESULT	SPK_AMT	%RECOVERY	QC LIMIT
Bromofluorobenzene	0.0342	0.0400	86	60-140

Notes:  
Parameter H-C Range  
Gasoline C6-C10  
Reported ND at RL quantitated per pattern recognition.

Detection limits are reported relative to sample result significant figures.  
Sample Amount : 5ml Final Volume : 5ml  
Prepared by : SCerva Analyzed by : SCerva

# QC SUMMARIES

METHOD 5030B/8015B  
TOTAL PETROLEUM HYDROCARBONS BY PURGE AND TRAP

```

=====
Client      : EUROFINS EATON ANALYTICAL   Date Collected: 04/06/22 15:29
Project     : 996836                      Date Received: 04/06/22
Batch No.   : 22D027                      Date Extracted: 04/06/22 15:29
Sample ID   : MBLK1W                      Date Analyzed: 04/06/22 15:29
Lab Samp ID: VG55D028                    Dilution Factor: 1
Lab File ID: UD06005A                    Matrix: WATER
Ext Btch ID: 22VG55D02                   % Moisture: NA
Calib. Ref.: UD06004A                    Instrument ID: 55
=====

```

PARAMETERS	RESULTS (mg/L)	RL (mg/L)	MDL (mg/L)		
GASOLINE	ND	0.020	0.010		
SURROGATE PARAMETERS	RESULT	SPK_AMT	%RECOVERY	QC LIMIT	
Bromofluorobenzene	0.0347	0.0400	87	60-140	

Notes:

Parameter H-C Range  
Gasoline C6-C10  
Reported ND at RL quantitated per pattern recognition.

Detection limits are reported relative to sample result significant figures.  
Sample Amount : 5ml Final Volume : 5ml  
Prepared by : SCerva Analyzed by : SCerva



EMAX QUALITY CONTROL DATA  
LAB CONTROL SAMPLE ANALYSIS

CLIENT : EUROFINS EATON ANALYTICAL  
PROJECT : 996836  
BATCH NO. : 22D027  
METHOD : 5030B/8015B

```

=====
MATRIX      : WATER                               % MOISTURE:NA
DILUTION FACTOR: 1                               1
SAMPLE ID   : MBLK1W                             LCS1W      LCD1W
LAB SAMPLE ID : VG55D02B                         VG55D02L   VG55D02C
LAB FILE ID  : UD06005A                         UD06006A   UD06007A
DATE PREPARED : 04/06/22 15:29                  04/06/22 16:06  04/06/22 16:43
DATE ANALYZED : 04/06/22 15:29                  04/06/22 16:06  04/06/22 16:43
PREP BATCH   : 22VG55D02                        22VG55D02   22VG55D02
CALIBRATION REF: UD06004A                       UD06004A   UD06004A
=====

```

ACCESSION:

PARAMETERS	MBResult (mg/L)	SpikeAmt (mg/L)	LCSResult (mg/L)	LCSRec (%)	SpikeAmt (mg/L)	LCDResult (mg/L)	LCDRec (%)	RPD (%)	QCLimit (%)	MaxRPD (%)
Gasoline	ND	0.500	0.439	88	0.500	0.467	93	6	60-130	30

SURROGATE PARAMETER	SpikeAmt (mg/L)	LCSResult (mg/L)	LCSRec (%)	SpikeAmt (mg/L)	LCDResult (mg/L)	LCDRec (%)	QCLimit (%)
Bromofluorobenzene	0.0400	0.0432	108	0.0400	0.0442	111	70-130

MB: Method Blank sample LCS: Lab Control Sample LCD: Lab Control Sample Duplicate

EMAX QUALITY CONTROL DATA  
MS/MSD ANALYSIS

CLIENT : EUROFINS EATON ANALYTICAL  
PROJECT : 996833  
BATCH NO. : 22D026  
METHOD : 50308/8015B

```

=====
MATRIX      : WATER                               % MOISTURE:NA
DILUTION FACTOR: 1                               1
SAMPLE ID   : 202204050422                       202204050422MSD
LAB SAMPLE ID : D026-01                           D026-01S
LAB FILE ID  : UD06012A                           UD06014A
DATE PREPARED : 04/06/22 19:46                     04/06/22 20:59
DATE ANALYZED : 04/06/22 19:46                     04/06/22 20:59
PREP BATCH   : 22VG55D02                           22VG55D02
CALIBRATION REF: UD06004A                           UD06004A
  
```

ACCESSION:

PARAMETERS	PSResult (mg/L)	SpikeAmt (mg/L)	MSResult (mg/L)	MSRec (%)	SpikeAmt (mg/L)	MSDResult (mg/L)	MSDRec (%)	RPD (%)	QCLimit (%)	MaxRPD (%)
Gasoline	ND	0.500	0.432	86	0.500	0.459	92	6	50-130	30

SURROGATE PARAMETER	SpikeAmt (mg/L)	MSResult (mg/L)	MSRec (%)	SpikeAmt (mg/L)	MSDResult (mg/L)	MSDRec (%)	QCLimit (%)
Bromofluorobenzene	0.0400	0.0417	104	0.0400	0.0436	109	60-140

PS: Parent Sample MS: Matrix Spike MSD: Matrix Spike Duplicate

LABORATORY REPORT FOR

EUROFINS EATON ANALYTICAL

996836

METHOD 3520C/8015B  
TOTAL PETROLEUM HYDROCARBONS BY EXTRACTION

SDG#: 22D027

CASE NARRATIVE

Client : EUROFINS EATON ANALYTICAL

Project: 996836

SDG : 22D027

METHOD 3520C/8015B  
TOTAL PETROLEUM HYDROCARBONS BY EXTRACTION

One(1) water sample was received on 04/06/22 to be analyzed for Total Petroleum Hydrocarbons by Extraction in accordance with Method 3520C/8015B and project specific requirements.

Holding Time

The sample was analyzed within the prescribed holding time.

Calibration

Multi-calibration points were generated to establish initial calibration (ICAL). ICAL was verified using a secondary source (ICV). Continuing calibration (CCV) verifications were carried out on a frequency specified by the project. All calibration requirements were within acceptance criteria. Refer to calibration summary forms of ICAL, ICV and CCV for details. MRL was analyzed as required by the project. Refer to MRL summary form for details.

Method Blank

Method blank was prepared and analyzed at the frequency required by the project. For this SDG, one(1) method blank was analyzed. DSD006WB - result was compliant to project requirement. Refer to sample result summary form for details.

Lab Control Sample

Lab control sample was prepared and analyzed at a frequency required by the project. For this SDG, one(1) LCS was analyzed. Percent recovery for Diesel was within LCS QC limits in DSD006WL. Refer to LCS summary form for details.

Matrix QC Sample

No matrix QC sample was provided on this SDG. One(1) set of MS/MSD was analyzed. Diesel was within MS QC limits in 22D026-01M/22D026-01S. Refer to Matrix QC summary form for details.

Surrogate

Surrogates were added on QC and field samples. All surrogate recoveries were within QC limits. Refer to sample result summary forms for details.

Sample Analysis

The sample was analyzed according to prescribed analytical procedures. Results were evaluated in accordance to project requirements. For this SDG, all quality control requirements were met.

LAB CHRONICLE  
TOTAL PETROLEUM HYDROCARBONS BY EXTRACTION

```

=====
Client      : EUROFINS EATON ANALYTICAL
Project    : 996836
=====
SDG NO.    : 22D027
Instrument ID : D5
=====

```

Client Sample ID	Laboratory Sample ID	Dilution Factor	% Moist	WATER			Extraction Date/Time	Sample Data FN	Calibration Data FN	Prep. Batch	Notes
				Analysis Date/Time	Extraction Date/Time	Sample Data FN					
MBLK1W	DSD006WB	1	NA	04/07/2214:06	04/06/2215:15	LD07010A	LD07004A	LD07004A	22DSD006W	Method Blank	
LCS1W	DSD006WL	1	NA	04/07/2214:24	04/06/2215:15	LD07011A	LD07004A	LD07004A	22DSD006W	Lab Control Sample (LCS)	
202204050426	D027-01	1	NA	04/07/2218:42	04/06/2215:15	LD07024A	LD07004A	LD07004A	22DSD006W	Field Sample	

```

=====
FN      - Filename
% Moist - Percent Moisture
=====

```

# **SAMPLE RESULTS**

METHOD 3520C/8015B  
TOTAL PETROLEUM HYDROCARBONS BY EXTRACTION

```

=====
Client      : EUROFINS EATON ANALYTICAL      Date Collected: 04/04/22 10:07
Project     : 996836                          Date Received: 04/06/22
Batch No.   : 22D027                          Date Extracted: 04/06/22 15:15
Sample ID   : 202204050426                    Date Analyzed: 04/07/22 18:42
Lab Samp ID: 22D027-01                        Dilution Factor: 1
Lab File ID: LD07024A                          Matrix: WATER
Ext Btch ID: 22DSD006W                        % Moisture: NA
Calib. Ref.: LD07004A                        Instrument ID: D5
=====

```

PARAMETERS	RESULTS (mg/L)	RL (mg/L)	MDL (mg/L)	
Diesel	ND	0.024	0.012	
Motor Oil	ND	0.047	0.024	
SURROGATE PARAMETERS	RESULT	SPK_AMT	%RECOVERY	QC LIMIT
Bromobenzene	0.461	0.470	98	60-130
Hexacosane	0.142	0.118	121	60-130

Notes:

Parameter H-C Range  
Diesel C10-C24  
Motor Oil C24-C36

Reported ND at RL quantitated per pattern recognition.

Detection limits are reported relative to sample result significant figures.

Sample Amount : 1060ml Final Volume : 5ml  
Prepared by : POrreto Analyzed by : SDeeso

# QC SUMMARIES



METHOD 3520C/8015B  
TOTAL PETROLEUM HYDROCARBONS BY EXTRACTION

```

=====
Client      : EUROFINS EATON ANALYTICAL   Date Collected: 04/06/22 15:15
Project     : 996836                      Date Received: 04/06/22
Batch No.   : 22D027                      Date Extracted: 04/06/22 15:15
Sample ID   : MBLK1W                      Date Analyzed: 04/07/22 14:06
Lab Samp ID: DSD006WB                    Dilution Factor: 1
Lab File ID: LD07010A                    Matrix: WATER
Ext Btch ID: 22DSD006W                   % Moisture: NA
Calib. Ref.: LD07004A                    Instrument ID: D5
=====

```

PARAMETERS	RESULTS (mg/L)	RL (mg/L)	MDL (mg/L)	
Diesel	ND	0.025	0.012	
Motor Oil	ND	0.050	0.025	
SURROGATE PARAMETERS	RESULT	SPK_AMT	%RECOVERY	QC LIMIT
Bromobenzene	0.426	0.500	85	60-130
Hexacosane	0.133	0.125	106	60-130

Notes:

Parameter H-C Range  
Diesel C10-C24  
Motor Oil C24-C36

Reported ND at RL quantitated per pattern recognition.

Detection limits are reported relative to sample result significant figures.

Sample Amount : 1000ml                      Final Volume : 5ml  
Prepared by : POrreto                        Analyzed by : SDeeso

EMAX QUALITY CONTROL DATA  
LAB CONTROL SAMPLE ANALYSIS

CLIENT : EUROFINS EATON ANALYTICAL  
PROJECT : 996836  
BATCH NO. : 22D027  
METHOD : 3520C/8015B

=====

MATRIX	: WATER	% MOISTURE:NA
DILUTION FACTOR:	1	1
SAMPLE ID	: MBLK1W	LCS1W
LAB SAMPLE ID	: DSD006WB	DSD006WL
LAB FILE ID	: LD07010A	LD07011A
DATE PREPARED	: 04/06/22 15:15	04/06/22 15:15
DATE ANALYZED	: 04/07/22 14:06	04/07/22 14:24
PREP BATCH	: 22DSD006W	22DSD006W
CALIBRATION REF:	LD07004A	LD07004A

ACCESSION:

PARAMETERS	MBResult (mg/L)	SpikeAmt (mg/L)	LCSResult (mg/L)	LCSRec (%)	QCLimit (%)
-----	-----	-----	-----	-----	-----
Diesel	ND	2.50	2.95	118	50-130

SURROGATE PARAMETERS	SpikeAmt (mg/L)	LCSResult (mg/L)	LCSRec (%)	QCLimit (%)
-----	-----	-----	-----	-----
Bromobenzene	0.500	0.468	94	60-130
Hexacosane	0.125	0.136	109	60-130

=====

MB: Method Blank sample    LCS: Lab Control Sample

EMAX QUALITY CONTROL DATA  
MS/MSD ANALYSIS

CLIENT : EUROFINS EATON ANALYTICAL  
PROJECT : 996833  
BATCH NO. : 22D026  
METHOD : 3520C/8015B

```

=====
MATRIX      : WATER                                % MOISTURE:NA
DILUTION FACTOR: 1                                1
SAMPLE ID   : 202204050422                        202204050422MSD
LAB SAMPLE ID : 22D026-01                          22D026-01S
LAB FILE ID  : LD07021A                            LD07022A
DATE PREPARED : 04/06/22 15:15                    04/06/22 15:15
DATE ANALYZED : 04/07/22 17:47                    04/07/22 18:24
PREP BATCH   : 22DSD006W                          22DSD006W
CALIBRATION REF: LD07004A                          LD07004A
=====

```

ACCESSION:

PARAMETERS	PSResult (mg/L)	SpikeAmt (mg/L)	MSResult (mg/L)	MSRec (%)	SpikeAmt (mg/L)	MSDResult (mg/L)	MSDRec (%)	RPD (%)	QCLimit (%)	MaxRPD (%)
Diesel	ND	2.62	3.07	117	2.58	2.93	114	5	50-130	30

SURROGATE PARAMETERS	SpikeAmt (mg/L)	MSResult (mg/L)	MSRec (%)	SpikeAmt (mg/L)	MSDResult (mg/L)	MSDRec (%)	QCLimit (%)
Bromobenzene	0.525	0.514	98	0.515	0.478	93	60-130
Hexacosane	0.131	0.151	115	0.129	0.143	111	60-130

PS: Parent Sample MS: Matrix Spike MSD: Matrix Spike Duplicate